

CAT CERULOPLASMIN ELISA

Life Diagnostics, Inc., Catalog Number: CER-8

INTRODUCTION

Ceruloplasmin, the major copper transport protein in blood, is an acute phase protein that is elevated in serum because of injury, infection or disease. Studies at Life Diagnostics, Inc. indicate that ceruloplasmin levels increase up to 8-fold during the acute phase response in cats. Ceruloplasmin is usually measured via its oxidase activity; a somewhat cumbersome method. This ELISA allows rapid measurement of ceruloplasmin in cat serum and plasma.

PRINCIPLE OF THE ASSAY

The assay uses affinity purified rat ceruloplasmin antibodies for solid phase (microtiter wells) immobilization and horseradish peroxidase (HRP) conjugated rat ceruloplasmin antibodies for detection. Standards and diluted samples are incubated in the microtiter wells for 45 minutes. The wells are subsequently washed. HRP conjugate is added and incubated for 45 minutes. This results in ceruloplasmin molecules being sandwiched between the immobilization and detection antibodies. The wells are then washed to remove unbound HRP-conjugate and TMB is added and incubated for 20 minutes. If ceruloplasmin is present a blue color develops. Color development is stopped by the addition of Stop solution, changing the color to yellow, and absorbance is measured at 450 nm. The concentration of ceruloplasmin is proportional to absorbance and is derived from a standard curve.

MATERIALS AND COMPONENTS

Materials provided with the kit:

- Ceruloplasmin antibody coated 96-well plate (12 x 8-well strips)
- HRP Conjugate, 11 ml
- Ceruloplasmin stock
- 20x Wash solution; TBS50-20, 50 ml
- 10x Diluent; YD25-10, 25 ml
- TMB, TMB11-1, 11 ml
- Stop solution, SS11-1, 11 ml

Materials required but not provided:

- Pipettors and tips
- Distilled or deionized water
- Polypropylene or glass tubes
- Vortex mixer
- Absorbent paper or paper towels
- Plate incubator/shaker
- Plate washer
- Plate reader capable of measuring absorbance at 450 nm.
- Curve fitting software

STORAGE

The kit should be stored at 2-8°C and the microtiter plate should be kept in a sealed bag with desiccant. The kit will remain stable for six months from the date of purchase.

GENERAL INSTRUCTIONS

1. All reagents should be allowed to reach room temperature before use.

2. Reliable and reproducible results will be obtained when the assay is carried out with a complete understanding of the instructions and with adherence to good laboratory practice.
3. The wash procedure is critical. Insufficient washing will result in poor precision and falsely elevated absorbance readings.
4. Laboratory temperature will influence absorbance readings. Our ELISA kits are calibrated using shaking incubators set at 150 rpm and 25°C. Performance of the assay at lower temperatures will result in lower absorbance values.

DILUENT PREPARATION

The diluent is provided as a 10x stock. Prior to use estimate the final volume of diluent required for your assay and dilute one volume of the 10x stock with nine volumes of distilled or deionized water.

WASH SOLUTION PREPARATION

The wash solution is provided as a 20x stock. Prior to use dilute the contents of the bottle (50 ml) with 950 ml of distilled or deionized water.

STANDARD PREPARATION

1. The cat ceruloplasmin stock is provided lyophilized stock¹. Add the volume of distilled or deionized water indicated on the vial label and mix gently until dissolved. The reconstituted standard should be aliquoted and frozen at -20°C after reconstitution if further use is intended.
2. Label 8 microcentrifuge tubes; 100, 50, 25, 12.5, 6.25, 3.13, 1.56 and 0.78 ng/ml.
3. In the tube labelled 100 ng/ml, prepare the 100 ng/ml standard as described on the stock vial label.
4. Dispense 250 µl of diluent into the tubes labelled 50, 25, 12.5, 6.25, 3.13, 1.56 and 0.78 ng/ml.
5. Prepare the 50 ng/ml standard by diluting and mixing 250 µl of the 100 ng/ml standard with 250 µl of diluent in the appropriate tube.
6. Similarly prepare the remaining standards by 2-fold serial dilution.

SAMPLE PREPARATION

Ceruloplasmin is present in cat serum at concentrations ranging from 100 to 800 µg/ml. To obtain values within the range of the standard curve we suggest that samples be diluted 10,000-fold using the following procedure.

1. Dispense 198 µl and 297 µl of diluent into separate tubes.
2. Pipette and mix 2.0 µl of the serum/plasma sample into the tube containing 198 µl of diluent. This provides a 100-fold diluted sample.
3. Mix 3.0 µl of the 100-fold diluted sample with the 297 µl of diluent in the second tube. This provides a 10,000-fold dilution of the sample.

¹ The standard is comprised of cat ceruloplasmin purified at Life Diagnostics, Inc., diluted in a stabilizing carrier protein matrix.

ASSAY PROCEDURE

1. Secure the desired number of 8-well strips in the holder. Unused strips should be stored in the re-sealed bag with desiccant at 2-8°C for future use.
2. Dispense 100 µl of standards and samples into the wells (we recommend that standards and samples be run in duplicate).
3. Incubate on an orbital micro-plate shaker at 150 rpm and 25°C for 45 minutes.
4. Empty and wash the microtiter wells 5x with 1x wash solution using a plate washer (400 µl/well).
5. Strike the wells sharply onto absorbent paper or paper towels to remove all residual droplets.
6. Add 100 µl of HRP-conjugate into each well.
7. Incubate on a plate shaker at 150 rpm and 25°C for 45 minutes.
8. Wash as detailed above.
9. Strike the wells sharply onto absorbent paper or paper towels to remove residual droplets.
10. Dispense 100 µl of TMB into each well.
11. Incubate on an orbital micro-plate shaker at 150 rpm at 25°C for 20 minutes.
12. After 20-minutes, stop the reaction by adding 100 µl of Stop solution to each well.
13. Gently mix. It is important to make sure that all the blue color changes to yellow.
14. Read absorbance at 450 nm with a plate reader within 5 minutes.


CALCULATION OF RESULTS

1. Using curve fitting software, construct a standard curve by plotting absorbance values of the standards versus log₁₀ of the concentration.
2. Fit the standard curve to a four-parameter logistic regression (4PL) equation (x axis = log₁₀ concentration) and determine the concentration of the samples from the standard curve (remember to derive the concentration from the antilog).
3. Multiply the derived concentration by the dilution factor to determine the actual concentration in the serum or plasma sample.
4. If the A₄₅₀ values of samples fall outside the standard curve, samples should be diluted appropriately and re-tested.

TYPICAL STANDARD CURVE

A typical standard curve is shown below. This curve is for illustration only and should not be used to calculate unknowns.

Ceruloplasmin (ng/ml)	Absorbance (450 nm)
100	3.527
50	2.342
25	1.408
12.5	0.835
6.25	0.534
3.13	0.334
1.56	0.238
0.78	0.209

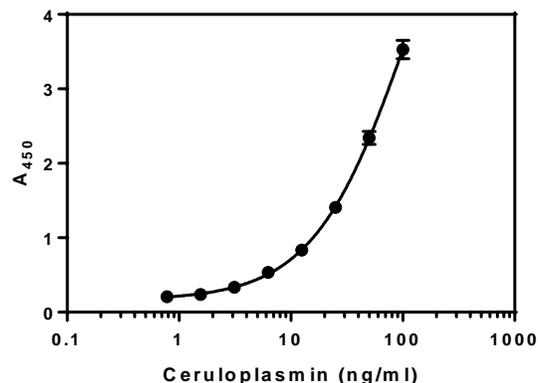

Rev 121217

For technical assistance please email us at techsupport@lifediagnosics.com