


RAT THIOSTATIN ELISA

Life Diagnostics, Inc., Catalog Number: THIO-2

INTRODUCTION

Thiostatin is a cysteine protease inhibitor that is also known as major acute phase protein (α 1-MAP).¹ In response to inflammation, serum levels of thiostatin increase as much as 20-fold.^{2,3} As shown in the figure below, studies at Life Diagnostics, Inc. found a significant increase in serum thiostatin in a rat arthritis model. Thiostatin is a useful biomarker of inflammation and disease in rats.

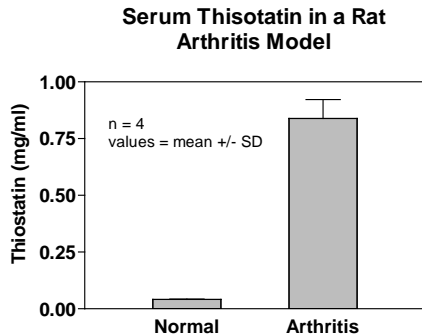

PRINCIPLE OF THE ASSAY

The assay uses affinity purified rat thiostatin antibodies for solid phase (microtiter wells) immobilization and horseradish peroxidase (HRP) conjugated rat thiostatin antibodies for detection. Standards and diluted samples are incubated in the microtiter wells for 45 minutes. The wells are subsequently washed. HRP conjugate is added and incubated for 45 minutes. This results in thiostatin molecules being sandwiched between the immobilization and detection antibodies. The wells are then washed to remove unbound HRP-conjugate and TMB is added and incubated for 20 minutes. If thiostatin is present a blue color develops. Color development is stopped by the addition of Stop solution, changing the color to yellow, and absorbance is measured at 450 nm. The concentration of thiostatin is proportional to absorbance and is derived from a standard curve.

MATERIALS AND COMPONENTS

Materials provided with the kit:

- Thiostatin antibody coated 96-well plate (12 x 8-well strips)
- HRP Conjugate, 11 ml
- Thiostatin stock (lyophilized)
- 20x Wash solution; TBS50-20, 50 ml
- 10x Diluent; YD25-10, 25 ml
- TMB, TMB11-1, 11 ml
- Stop solution, SS11-1, 11 ml

Materials required but not provided:

- Pipettors and tips
- Distilled or deionized water
- Polypropylene or glass tubes
- Vortex mixer
- Absorbent paper or paper towels
- Plate incubator/shaker
- Plate washer
- Plate reader capable of measuring absorbance at 450 nm.
- Curve fitting software

STORAGE

The kit should be stored at 2-8°C and the microtiter plate should be kept in a sealed bag with desiccant. Kits will remain stable for six months from the date of purchase.

GENERAL INSTRUCTIONS

1. All reagents should be allowed to reach room temperature before use.
2. Reliable and reproducible results will be obtained when the assay is carried out with a complete understanding of the instructions and with adherence to good laboratory practice.
3. The wash procedure is critical. Insufficient washing will result in poor precision and falsely elevated absorbance readings.
4. Laboratory temperature will influence absorbance readings. Our ELISA kits are calibrated using shaking incubators set at 150 rpm and 25°C. Performance of the assay at lower temperatures will result in lower absorbance values.

DILUENT PREPARATION

The diluent is provided as a 10x stock. Prior to use estimate the final volume of diluent required for your assay and dilute one volume of the 10x stock with nine volumes of distilled or deionized water.

WASH SOLUTION PREPARATION

The wash solution is provided as a 20x stock. Prior to use dilute the contents of the bottle (50 ml) with 950 ml of distilled or deionized water.

STANDARD PREPARATION

1. The rat thiostatin stock is provided lyophilized. Add the volume of distilled or de-ionized water indicated on the vial label and mix gently until dissolved.
2. Label 7 polypropylene or glass tubes as 75, 37.5, 18.75, 9.38, 4.67, 2.34 and 1.17 ng/ml.
3. In the tube labeled 75 ng/ml prepare the 75 ng/ml standard as detailed on the stock vial label.
4. Dispense 250 μ l of diluent into the tubes labeled 37.5, 18.75, 9.38, 4.67, 2.34 and 1.17 ng/ml.
5. Prepare the 37.5 ng/ml standard by mixing 250 μ l of the 75 ng/ml standard with 250 μ l of diluent in the tube labeled 37.5 ng/ml.
6. Similarly prepare the remaining standards by two-fold serial dilution.

The reconstituted stock remains stable for at least 1 day at 2-8°C but should be aliquoted and frozen at -20°C if use beyond this time is intended.

SAMPLE PREPARATION

We found that thiostatin was present in normal rat serum at a concentration of approximately 50 μ g/ml. Levels up to 1 mg/ml were found in serum from rats with arthritis. To obtain values within range of the standard curve, we suggest that samples initially be diluted 10,000-fold using the following procedure for each sample to be tested:

1. Dispense 495 μ l and 297 μ l of 1x diluent into separate tubes.

- Pipette and mix 5.0 μl of the serum/plasma sample into the tube containing 495 μl of 1x diluent. This provides a 100-fold dilution.
- Mix 3.0 μl of the 100-fold diluted sample with the 297 μl of diluent in the second tube. This provides a 10,000-fold dilution.

ASSAY PROCEDURE

- Secure the desired number of 8-well strips in the holder. Unused strips should be stored in the re-sealed bag with desiccant at 4°C for future use.
- Dispense 100 μl of standards and samples into the wells (we recommend that standards and samples be run in duplicate).
- Incubate on an orbital micro-plate shaker at 150 rpm and 25°C for 45 minutes.
- Empty and wash the microtiter wells 5x with 1x wash solution using a plate washer (400 μl /well).
- Strike the wells sharply onto absorbent paper or paper towels to remove all residual droplets.
- Add 100 μl of HRP-conjugate into each well.
- Incubate on a plate shaker at 150 rpm and 25°C for 45 minutes.
- Wash as detailed above.
- Strike the wells sharply onto absorbent paper or paper towels to remove residual droplets.
- Dispense 100 μl of TMB into each well.
- Incubate on an orbital micro-plate shaker at 150 rpm at 25°C for 20 minutes.
- After 20-minutes, stop the reaction by adding 100 μl of Stop solution to each well.
- Gently mix. It is important to make sure that all the blue color changes to yellow.
- Read absorbance at 450 nm with a plate reader within 5 minutes.


CALCULATION OF RESULTS

- Using curve fitting software, construct a standard curve by plotting absorbance values of the standards versus \log_{10} of the concentration.
- Fit the standard curve to a four-parameter logistic regression (4PL) equation (x axis = \log_{10} concentration) and determine the concentration of the samples from the standard curve (remember to derive the concentration from the antilog).
- Multiply the derived concentration by the dilution factor to determine the actual concentration in the serum or plasma sample.
- If the A_{450} values of samples fall outside the standard curve, samples should be diluted appropriately and re-tested.

TYPICAL STANDARD CURVE

A typical standard curve is shown below. This curve is for illustration only and should not be used to calculate unknowns. A standard curve should be run in each experiment.

Thiostatin (ng/ml)	Absorbance (450 nm)
75	3.702
37.5	2.959
18.75	1.863
9.38	1.077
4.67	0.588
2.34	0.336
1.17	0.210

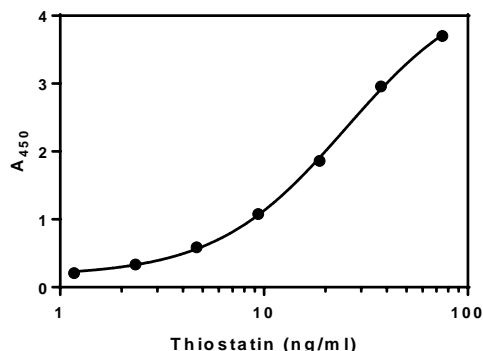

REFERENCES

- KP Anderson and EC Heath. The relationship between rat major acute phase protein and the kininogens. *J Biol Chem.* 260:12065-12071 (1985)
- J Urban, et al. A rat serum glycoprotein whose synthesis rate increases greatly during inflammation. *J Biol Chem.* 254:10565-10568 (1979)
- I Miller, et al. Proteins of rat serum: III. Gender-related differences in protein concentration under baseline conditions and upon experimental inflammation as evaluated by two-dimensional electrophoresis. *Electrophoresis.* 20:836-845 (1999)

Rev 121917

For technical assistance please email us at
techsupport@lifediagnosics.com